

This Page Is Inserted by IFW Operations  
and is not a part of the Official Record

## **BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

**IMAGES ARE BEST AVAILABLE COPY.**


**As rescanning documents *will not* correct images,  
please do not report the images to the  
Image Problem Mailbox.**





## INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

<b>(51) International Patent Classification:</b> A61L 31/08, A61F 2/06, A61K 51/12, A61L 31/16, A61L 31/18	<b>A1</b>	<b>(11) International Publication Number:</b> <b>WO 00/12147</b> <b>(43) International Publication Date:</b> 09 March 2000 (09.03.2000)
<b>(21) International Application Number:</b> PCT/US99/19697 <b>(22) International Filing Date:</b> 31 August 1999 (31.08.1999) <b>(30) Priority Data:</b> 09/145,707 02 September 1998 (02.09.1998) US <b>(60) Parent Application or Grant</b> SCIMED LIFE SYSTEMS, INC. [/]; (). YANG, Dachuan [/]; (). WANG, Lixiao [/]; (). ANDERSON, William, E., II; ().	<b>Published</b>	
<b>(54) Title: DRUG DELIVERY DEVICE FOR STENT</b> <b>(54) Titre: SYSTEME D'ADMINISTRATION DE MEDICAMENTS POUR STENT</b>  <b>(57) Abstract</b> <p>A device adapted for mounting on a stent, the device comprising a sheath being made of polymeric material that includes drugs such as pharmaceutical agent(s) or radioactive agent(s) for delivery to an implant site. The sheath includes a main body of a generally tubular shape, and may include mounting means for attaching same to the stent. The device may have a slit therein, and may comprise a helical coil, a cylinder or any other suitable shape or design which fits a particular stent. The sheath may include a coating or coatings thereon containing drugs, surgical adhesives or a combination thereof.</p> <b>(57) Abrégé</b> <p>L'invention concerne un dispositif conçu pour être monté sur un stent. Ce dispositif comprend une gaine en matériau polymère contenant des médicaments, par exemple un ou plusieurs agent(s) pharmaceutiques, devant être administrés sur le site d'implantation. Cette gaine comprend un élément principal de forme sensiblement tubulaire et peut comprendre des moyens de fixation permettant de la fixer sur le stent. Le dispositif peut comprendre une fente ainsi qu'un enroulement hélicoïdal, un cylindre ou toute autre forme ou structure adaptée à un stent particulier. La gaine peut en outre comprendre une ou plusieurs couches de revêtement contenant des médicaments, des adhésifs chirurgicaux ou une combinaison des deux.</p>		

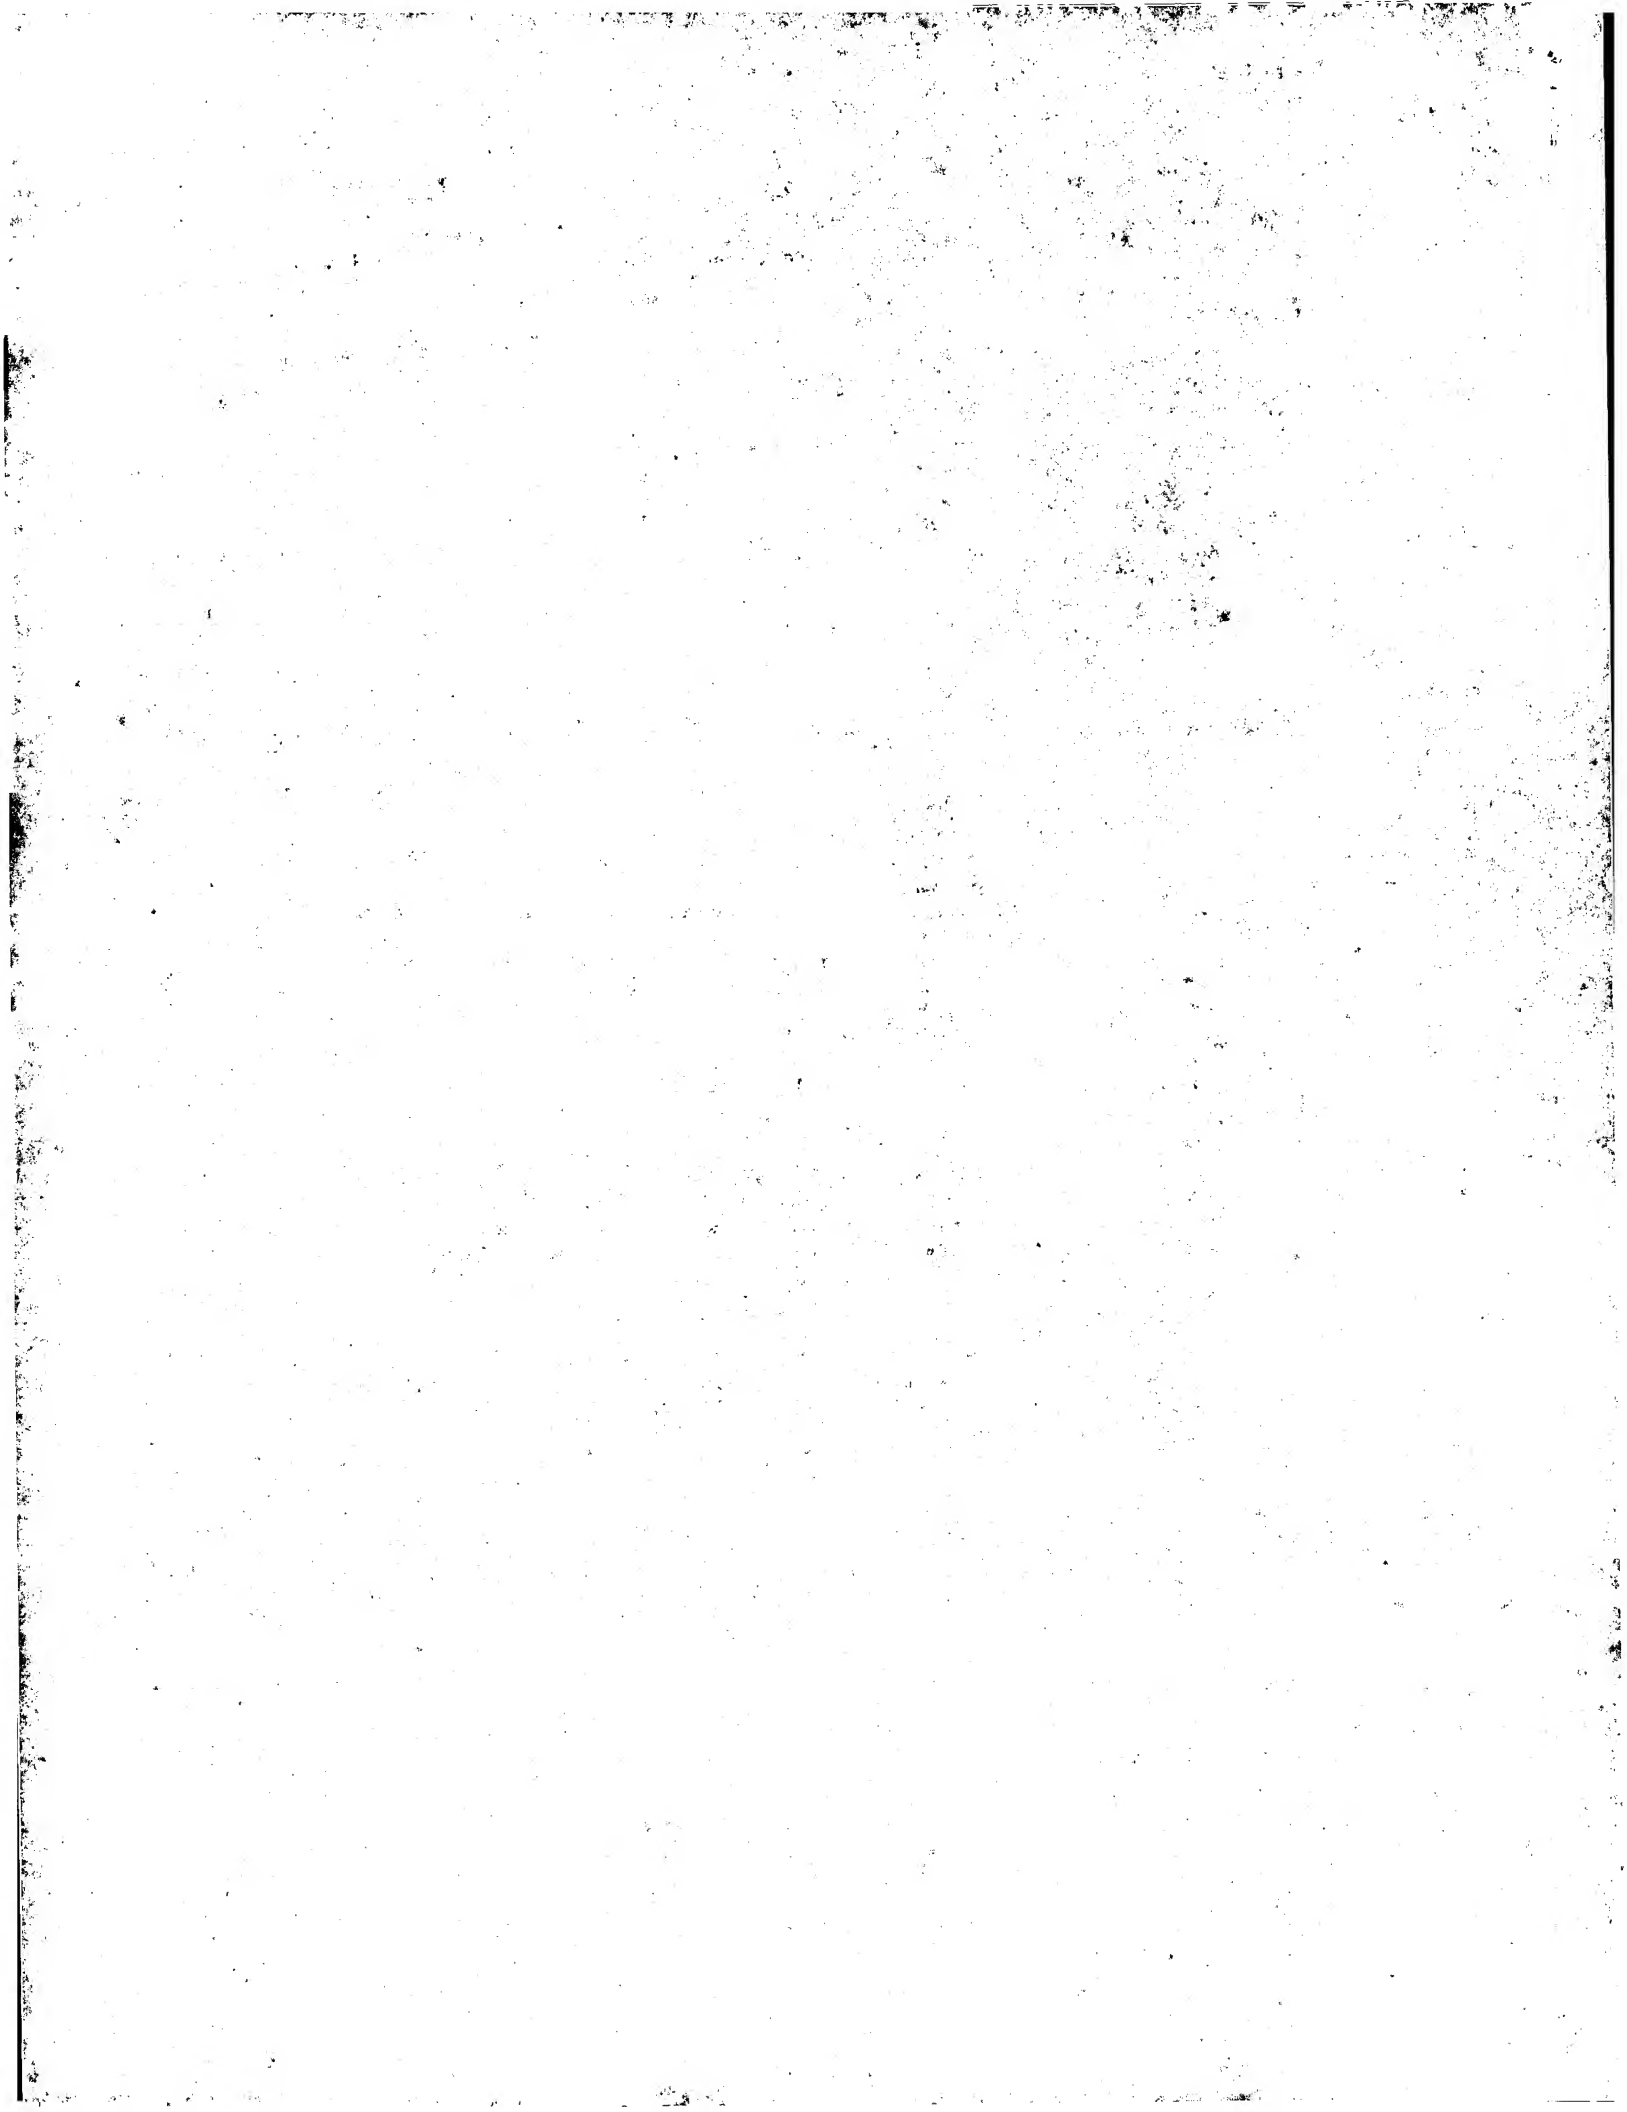

PCT

WORLD INTELLECTUAL PROPERTY ORGANIZATION  
International Bureau



INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification <sup>7</sup> : A61L 31/08, 31/16, 31/18, A61K 51/12, A61F 2/06		A1	(11) International Publication Number: WO 00/12147 (43) International Publication Date: 9 March 2000 (09.03.00)
(21) International Application Number: PCT/US99/19697 (22) International Filing Date: 31 August 1999 (31.08.99) (30) Priority Data: 09/145,707 2 September 1998 (02.09.98) US (71) Applicant: SCIMED LIFE SYSTEMS, INC. [US/US]; One Scimed Place, Maple Grove, MN 55311-1566 (US). (72) Inventors: YANG, Dachuan; 11274 49th Avenue North, 55442 Plymouth (US). WANG, Lixiao; 12822 86th Place North, Maple Grove, MN 44369 (US). (74) Agent: ANDERSON, William, E., II; Vidas, Arrett & Steinkraus, 6109 Blue Circle Drive, Suite 2000, Min- netonka, MN 55343-9131 (US).		(81) Designated States: CA, JP, European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE).  Published With international search report. Before the expiration of the time limit for amending the claims and to be republished in the event of the receipt of amendments.	
(54) Title: DRUG DELIVERY DEVICE FOR STENT			
(57) Abstract			
<p>A device adapted for mounting on a stent, the device comprising a sheath being made of polymeric material that includes drugs such as pharmaceutical agent(s) or radioactive agent(s) for delivery to an implant site. The sheath includes a main body of a generally tubular shape, and may include mounting means for attaching same to the stent. The device may have a slit therein, and may comprise a helical coil, a cylinder or any other suitable shape or design which fits a particular stent. The sheath may include a coating or coatings thereon containing drugs, surgical adhesives or a combination thereof.</p>			

**FOR THE PURPOSES OF INFORMATION ONLY**

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece			TR	Turkey
BG	Bulgaria	HU	Hungary	ML	Mali	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MN	Mongolia	UA	Ukraine
BR	Brazil	IL	Israel	MR	Mauritania	UG	Uganda
BY	Belarus	IS	Iceland	MW	Malawi	US	United States of America
CA	Canada	IT	Italy	MX	Mexico	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NE	Niger	VN	Viet Nam
CC	Congo	KE	Kenya	NL	Netherlands	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NO	Norway	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	NZ	New Zealand		
CM	Cameroon			PL	Poland		
CN	China	KR	Republic of Korea	PT	Portugal		
CU	Cuba	KZ	Kazakhstan	RO	Romania		
CZ	Czech Republic	LC	Saint Lucia	RU	Russian Federation		
DE	Germany	LI	Liechtenstein	SD	Sudan		
DK	Denmark	LK	Sri Lanka	SE	Sweden		
EE	Estonia	LR	Liberia	SG	Singapore		

**DRUG DELIVERY DEVICE FOR STENT****BACKGROUND OF THE INVENTION**

This invention relates to a device for providing mechanical support to a vessel lumen of a living being. This invention also relates to the delivery of materials which prevent restenosis of a vessel.

A variety of medical situations requires the use of a mechanism to expand and support a constricted vessel and to maintain an open passageway through the vessel. A few examples of such situations following angioplasty include holding a dissection in place, preventing closure during spasm, and preventing acute closure due to thrombosis. In these situations, devices, commonly known as stents, are useful to maintain the patency of body passages, to prevent stenosis of a dilated vessel, to eliminate the danger of occlusion caused by "flaps" resulting from intimal tears that may be associated with angioplasty, or to hold two ends of a vessel in place.

Stents are generally tubular in configuration, open ended and are expandable between a generally unexpanded insertion diameter and an expanded implantation diameter. Stents are commonly placed or implanted by a mechanical transluminal procedure.

Specifically, U.S. Patent 4,733,665 to Palmaz discloses a number of stent configurations for implantation with the aid of a catheter. U.S. Patent 5,019,090 to Pinchuk discloses a generally cylindrical stent and technique for implanting it using a deflated balloon catheter to position the stent. U.S. Patents 4,503,569 to Dotter and 4,512,338 to Balko et al. disclose a spring stent and a shape memory alloy stent. There are also self-expanding stents such as those described in U.S. Patents 4,732,152 to Wallsten et al. and 4,848,343 to Wallsten et al. All of these patents are hereby incorporated by reference.

Stents have been made using materials of varied composition and conformation. McGreevy et al U.S. Patents 4,690,684 and 4,770,176 describe a meltable stent that is inserted into the interior of the ends of a blood vessel during anastomosis. Anastomosis refers to the surgical or physical connection of two tubular structures, such as veins or arteries. The stent is made of blood plasma, which is biologically compatible with the living being and which melts rapidly in response to heat.

Fischell et al., in U.S. Patent 4,768,507 describe an intravascular stent which is an unrestrained coil spring having an outside diameter of 2 to 12 millimeters and a length of 5 to 25 millimeters. The materials of construction are stainless steel, and a

## Description

5

10

15

20

25

30

35

40

45

50

55



5 titanium alloy. Decreased thrombogenicity is achievable by coating the outside of the coil with a non-thrombogenic material such as ULTI carbon.

10 Leeven et al., in U.S. Patent 4,820,298 describe a stent having a flexible tubular body made from a thermal plastic to the form of a helix. Polyester and  
5 polycarbonate copolymers are selected as particularly desirable materials.

15 Wolff et al., in U.S. Patent 4,830,003 describe a stent made from wires formed into a cylinder. The wires are made of a biocompatible metal. Biocompatible metals include 300 series stainless steels such as 316 LSS, as well as platinum and  
platinum-iridium alloys, cobalt-chromium alloys such as MP35N, and unalloyed titanium.

20 Wiktor in U.S. Patent 4,886,062 describes a stent made from low memory metal such as a copper alloy, titanium, or gold. The stent is preformed into a two-dimensional zig-zag form creating a flat expandable band.

25 Gianturco in U.S. Patent 4,907,336 describes a wire stent having a cylindrical shape that results from an expandable serpentine configuration. Malleable materials of construction are preferably included from the group of annealed stainless  
15 steels, tungsten and platinum.

30 Goldberg et al, in Canadian Application 2,025,626, describes a bio-degradable infusion stent used to treat ureteral obstructions. The application describes an extruded material of construction made of epsilon-caprolactone (15-25% w/w of  
20 terpolymer composition); glycoside (5-50% w/w) and L(-)lactide (45-85% w/w). This material was described as having a minimum tensile strength of at least 500 pounds per square inch, preferably 650 psi; elongation of greater than 10%, preferably greater than  
35 100%; and Shore A hardness equal to 50-100%, preferably 75-95%. The Goldberg et al patent application describes a method for incorporating radiopaque materials such as  
40 25 barium sulfate into the polymer in amounts ranging from 5-30%. The mechanism of biodegradation is described as hydrolysis resulting in degradable products excreted in urine or reabsorbed into tissues. The duration of functional life of the stent is estimated at about  
3-7 weeks.

45 Wilcoff in U.S. Patent 4,990,155 describes a plastic stent having an  
30 inherently expandable coil conformation. The "inherency" results from an elastic memory conferred by electron beam radiation imparting cross-linkages that provide an inherent  
50 tendency to return to a given diameter after any distortion. Materials of construction

5 include high density polyethylene. Optionally, this material is compounded with an anti-coagulant and/or an x-ray opaque material such as bismuth-sub-carbonate.

10 Sigwart, Canadian Patent Application 2,008,312, describes a stent made from a malleable flat sheet having a reticulated pattern. The reticulated pattern includes  
5 non-deformable squares or diamonds. The stent is made by rolling the sheet and locking the sheet into a spiral having a small diameter. The sheet is locked into a spiral by a tie interwoven into the reticulated pattern. Once inserted into the lumen of a vessel, the spiral  
15 is expanded and held in place by flaps integrated into the outer body of the stent.

Shockley et al., in U.S. Patent 4,994,033, describe a drug delivery dilatation  
10 catheter having three flexible, plastic tubes concentrically arranged relative to each other. The outermost sleeve of this catheter contains microholes for drug delivery. These  
20 microholes are made with a laser beam. Drugs that can be delivered by this system include aspirin, persantin, heparin, and prostaglandins. Drugs are delivered when externally applied pressure causes the innermost sleeve to balloon out. The drug is then forced  
25 through the microholes to spray and to treat a lesion.

There are also stents which deliver agents or drugs to blood passing through  
30 the vein or artery that are generally beneficial to the recipient. In addition, stents can deliver drugs or biologically active agents at a controlled rate to blood passing through the vessel lumen as well as to the vessel wall. Silvestrini in U.S. Patent 5,234,456 describes  
20 a hydrophilic stent comprising a wall structure where at least a portion thereof is a hollow wall in which a hydrophilic material for drug delivery is placed. U.S. Patent 5,443,458 to  
35 Eury et al., is directed to a multilayer laminated resorbable stent having a structural layer and additional layers stated to release drugs at predictable rates. Froix in U.S. 5,258,020 describes a self-restrained stent with an elastic memory, the stent optionally being  
40 formulated to provide for drug administration.

It is known that when stents are expanded to their implantation diameter the  
ends of the stent may press into the vessel or cavity walls, especially the distal end of the  
45 stent. The sharp or pointed edges and ends of some stents may then damage the walls. Once damage has occurred, there is a likelihood that restenosis will occur at these points  
30 where the stents ends and edges have penetrated or pressed against the walls.

Restenosis occurs in a number of cases where a stent has been used. Tearing  
50 of the wall of the passage or injury of the endothelial cell layer are possible causes of the

5 restenosis. The torn wall or flap usually is the source of the blockage. When the wall is  
torn, a flap of tissue is created, which falls into the passage and blocks it. It is then  
10 necessary to perform another procedure to remove the blockage and generally, another  
stent is needed to open the vessel or other passage. Metal stents are known to cause 10%  
5 to 30% or more restenosis in application.

Therefore, it desirable to utilize a stent which reduces the chances of a  
15 damaged vessel wall or body passage which leads to further problems and further necessary  
procedures. However, current stents are not designed to reduce the occurrence of cutting  
of vascular passages or the like.

10 U.S. Patent Application No. 09/072,944, incorporated herein by reference,  
is directed to a stent having at least one smooth end. The stent may include a coating or  
20 coatings on one or both end portions to provide a smooth finish to reduce possible damage  
to body passages when the stent is deployed and delivered. The stent may also contain  
drugs or surgical adhesives or a combination thereof in or on the coated portion of the stent.  
25 The stent may also be of the type where the materials of the stent may be treated to have  
a smooth flexible end or ends. The stent may also be of a configuration such that at least  
one end is more flexible than the middle portion of the stent.

30 U.S. Patent Application No. 08/874,190, incorporated herein by reference,  
discloses a polymeric layered stent characterized in that it includes a multilayered material  
20 comprised of an inner polymer layer and an overlying outer polymer layer. The self-  
expanding or balloon expandable stent disclosed therein is provided in two forms, one  
35 including inner and outer polymeric layers, and another comprising a prior art stent  
provided with polymeric layer(s) coated thereon.

40 While U.S. Applications 09/072,944 and 08/874,190 are directed in part to  
25 this need, there still exists a need for a means for delivering drugs or biologically active  
agents which assist in preventing restenosis, which can be easily mounted on an existing  
stent prior to implantation.

#### 45 SUMMARY OF THE INVENTION

Accordingly, it is an object of the present invention is to provide a polymeric  
30 device adapted for mounting onto a stent. The device of polymeric material may comprise  
a sheath or sleeve that is cylindrical, a helical coil, or any other suitable shape or design  
50 which fits a particular stent. The stent may be metallic or non-metallic, or alternatively a

5 combination of metallic and non-metallic materials. An example of a preferred stent for  
use with the device of the present invention is the NIR stent, set forth in U.S. Patent  
5,733,303, incorporated herein by reference. In addition, the device may be used with a  
10 stent as set forth in U.S. Application No. 08/874,190, incorporated herein by reference.

5 The device may be of a biocompatible material and may be either  
biodegradable or non-biodegradable. The device may also be water soluble. It may contain  
pharmaceutical agent(s) or radioactive agent(s). The device is adapted for mounting onto  
15 a stent prior to use for insertion into a lumen of a vessel in a living being, and may be  
expanded with the stent. The device is optionally biodegradable, and may be made from  
10 at least one biodegradable material that is also biocompatible and includes a drug which is  
released into the lumen of the vessel at a rate controlled by the rate of degradation of the  
20 biodegradable material.

Generally, any prior art stent may be improved by providing it with the  
device of the present invention. The use of this inventive device with an existing stent  
25 provides a simple method for reducing restenosis.

#### BRIEF DESCRIPTION OF THE DRAWINGS

Figure 1 is an enlarged perspective view of a device according to the present  
30 invention;

Figures 2a and 2b are perspective views of an alternative embodiment of the  
20 device of the present invention;

Figure 3 is a perspective view of an alternative embodiment of the device of  
35 the present invention;

Figure 4 is a perspective view of an alternative embodiment of the device  
40 of the present invention;

Figure 5 is a cross section taken along the line 5-5 of Figure 4;

Figure 6 is a perspective view of an alternative embodiment of a device  
25 according to the present invention;

Figure 7 is a cross section taken along line 7-7 of Figure 6;

Figure 8 is a perspective view of an alternative embodiment of a device  
45 according to the present invention;

Figure 9 is a fragmentary perspective view of the sheath as shown in Figure  
30 8 mounted on a stent;

Figure 10 is a fragmentary perspective view as in Figure 9 showing the stent and sheath after expansion of the stent; and

Figure 11 is a fragmentary side elevational view with parts broken away of the stent with the sheath of the present invention in an implanted site.

#### DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENTS

The present invention is a polymeric device adapted for mounting onto a stent. Referring to Figures 1-4, the device may be a sheath as shown generally at 10. Sheath 10 has a proximal end 12, a distal end 14, an interior surface 16 and an exterior surface 18.

As shown at Figures 2a, 2b and 3, sheath 10 may have a slit 15 therein extending from proximal end 12 to distal end 14. As shown at Figure 2a, slit 15 is a longitudinal slit 15a. Figure 2b shows the same sheath in a compressed configuration it may take on prior to being mounted on a stent. Alternatively, slit 15 may be a helical slit 15b, as shown at Figure 3.

Referring to Figure 4, sheath 10 may be provided with perforations 17 therethrough. In addition, sheath 10 may comprise multiple layers, for example as shown in cross section at Figure 5 having two layers. Alternatively, sheath 10 may comprise a plurality of layers. Referring to Figures 6-7, sheath 10 may be shaped like a spring, which spring may optionally be formed from a tubular member, as exemplified by the cross section at Figure 7.

Referring now to Figures 8-10, a sheath comprising a helical coil is shown. Figure 8 is a perspective view of sheath 10. At Figure 9, a partial section view of sheath 10 mounted on a stent 20 is shown prior to implantation and expansion. Stent 20 includes a generally tubular main body 21, a proximal end 22 (not shown in this view), a distal end 24 (not shown in this view), an interior surface 26 and an exterior surface 28. Prior to implantation, sheath 10 is mounted on stent 20 such that the exterior surface 28 of main body 21 faces the interior surface 16 of sheath 10.

In use, sheath 10 is placed on the outer surface 24 of stent 20 prior to implantation thereof. Sheath 10 may be held on stent 20 by any suitable means including compressive force, glue, a protective sheath, socks or the like.

The compressive force may be supplied by the sheath itself, the stent or both. The glue is preferably a biocompatible glue such as fibrin, collagen or gelatin. Any

appropriate bioadhesive may be used. For example, the following bioadhesives may be used singly or in combination:

cyanoacrylate: ethyl cyanoacrylate, butyl cyanoacrylate, octyl cyanoacrylate, hexyl cyanoacrylate;

fibrin glue: fibrinogen/thrombin/Factor XIII/calcium as catalyst  
gelatin-resorcinol-formol (GRF) glue: formed from gelatin, resorcinol and water in the presence of formaldehyde, glutaraldehyde and heat (45°C);

mussel adhesive protein, prolamine gel and transforming growth factor beta(TGF-B);

polyacrylic acid, modified hydrocellulose, hydroxypropylmethyl cellulose, hydroxypropylcellulose, carboxymethyl cellulose, sodium alginate, gelatin, pectin, polyvinylpyrrolidone, polyethylene glycol, aldehyde relative multifunctional chemicals, polyallylsaccharose, and polypeptides.

A protective sheath may also be used to secure sheath 10 to stent 20. A sheath or sheaths as disclosed in U.S. Application Nos. 08/812,351 and 09/034,434, incorporated herein by reference, may be used, but would be retained over sheath 10 in use.

At least one sock covering a portion of sheath 10 over stent 20 may also be used. Such a retaining device as is disclosed in U.S. Application No. 08/917,027, incorporated herein by reference, may be used.

One use of the sheath of the present invention is to allow physicians to add it to any stent and delivery system they already have. The sheath may therefore be provided as a stand alone device.

Stent 20 with sheath 10 mounted thereto is positioned at the inner surface wall 34 of the vessel 32 by radially compressing the stent with sheath to a tubular diameter less than the diameter of the vessel 32 and moving stent 20 to a desired site within vessel 32. Stent 20 is implanted in the known manner depending upon its type. For example, a self expanding stent would be released from compression so that the stent can radially spring out to abut against the inner surface wall 34 of vessel 32. The stent may also be of the balloon expandable type. In any case, sheath 10 is adapted for mounting onto stent 20 and expansion therewith. Figure 10 shows sheath 10 after expansion of stent 20.

At Figure 11, sheath 10 and stent 20 are shown in an implanted site, in the lumen 30 of a tubular vessel 32 in a body. Upon implantation, the exterior surface 18 of

5 sheath 10 faces an inner surface wall 34 of the vessel 32. Stent 20 provides mechanical support to tubular vessel 32 in a living being. The stent strengthens the area of vessel 32 in which it is implanted. Sheath 10 releases a pharmaceutical agent or radioactive agent  
10 into lumen 30 of tubular vessel 32. The rate of release may vary.

5 The present invention may be used with any stent. Such a stent may range from 1 millimeter in diameter to 50 millimeters in diameter and from 1 millimeter in length to 50 millimeters in length. The size of the stent is dictated by the lumen of the vessel to  
15 which the stent is placed. Tubular main body 21 suitably has a length of up to approximately 5 centimeters.

10 Sheath 10 may be of any size suitable for use with a stent being implanted.  
20 Many suitable materials may be used to form the sheath 10 of the present invention. For example, hydrophilic polymers, copolymers (block or graft) or their cross-linked versions (e.g. hydrogels), may be used, the polymers including poly(hydroxyethyl methacrylate) and derivatives; poly(vinyl alcohol); polyethylene oxide; poly(propylene  
25 oxide); polyacrylamides; polyacrylic acid; polymethacrylic acid; poly(N-vinyl-2-pyrrolidone); hydrophilic polyurethanes; poly(amino acid); water soluble cellulosic polymers (sodium carboxymethyl cellulose, hydroxyethyl cellulose, for example);  
30 collagens; carrageenan; alginate; starch; dextrin; and gelatins.

The device of the present invention may be made of biodegradable polymers  
20 including poly(lactide); poly(glycolide); polydioxanone(PDS); polycaprolactone; polyhydroxybutyrate(PHBT); poly(phosphazene); poly(phosphate ester); poly(lactide-co-glycolide); poly(glycolide-co-trimethylene carbonate); poly(glycolide-co-caprolactone);  
35 polyanhydrides; collagen or other connective proteins or natural materials, hyaluronic acid, adhesive proteins, co-polymers of these materials as well as composites or combinations thereof and combinations of other biodegradable polymers.  
40 25

In addition, the device of the present invention may be made of biodegradable materials that are also biocompatible. By biodegradable is meant that a material will undergo breakdown or decomposition into harmless compounds as part of a  
45 normal biological process. The device may also include bioactive agents which permit  
30 endothelial cells to grow on the device and the stent. It is believed that the endothelial cell growth will encapsulate particles of the stent during biodegradation that would otherwise  
50 come loose and form emboli in the blood stream.

5 Suitable biodegradable materials for the device of the present invention include polylactic acid, polyglycolic acid, collagen or other connective proteins or natural  
10 materials, polycaprolactone, hyaluronic acid, adhesive proteins, co-polymers of these materials as well as composites and combinations thereof, and combinations of other  
5 biodegradable polymers. Biodegradable glass or bioactive glass is also a suitable biodegradable material for use in the present invention. Preferably the materials have been  
15 accepted by the U.S. Food and Drug Administration.

One advantage of using a variety of biodegradable materials within the sheath is control of degradation. Biodegradable materials degrade at different rates, ranging  
10 from days or weeks to several years. Consequently, the presence of different biodegradable materials in the stent permits the sheath to degrade in a predictable manner. The device  
20 may further be coated with a biodegradable film layer.

Where sheath 10 is of a biodegradable material, the rate of release of the pharmaceutical agent or radioactive agent will be controlled by the rate of degradation of  
25 the biodegradable materials.

Further, the device of the present invention may be made of nonbiodegradable biocompatible materials such as polytetrafluoroethylene(PTFE);  
30 polyurethanes; polyamides; polyesters; polyethers; polyketones; polyether ester elastomers; polyether amide elastomers; polyacrylate-based elastomers; polyethylene; and  
20 polypropylene.

These lists are exemplary only. Any appropriate material may be used.

35 The sheath of the present invention includes pharmaceutical agent(s) and/or radioactive agent(s) or other biologically active materials. Where the sheath is biodegradable, these drugs, pharmaceutical agents, radioactive agents or biologically active  
40 materials are contained within the biodegradable materials of which the stent is composed. As the sheath biodegrades, drugs are released into the surrounding tissue or to the  
25 bloodstream. Thus, the rate of drug release is controlled by the rate of degradation of the biodegradable materials. A material that degrades rapidly will release the drug faster than  
45 a material that degrades slowly.

30 Drugs are incorporated into the biodegradable sheath using techniques known in the art. The techniques include simple mixing or solubilizing with polymer



5 solutions, dispersing into the biodegradable polymer during the formation of the sheath, or coating onto an already formed sheath.

10 Where the sheath has a film added thereto, drugs can be incorporated into the film by methods such as melting or solvation. Alternatively, biologically active agents  
5 are incorporated into the film layer by entrapment between such layer and the surface of biodegradable material sandwiched together, thereby further promoting release of the drugs or agents in a controllable manner.

15 The drugs or other biologically active materials incorporated into the sheath of the present invention perform a variety of functions. The functions include but are not  
20 limited to an anti-clotting or anti-platelet function and preventing smooth muscle cell growth on the inner surface of the vessel to reduce the chance of in-stent restenosis. The drugs include but are not limited to drugs that inhibit or control the formation of thrombus or thrombolytics such as heparin or heparin fragments, aspirin, coumadin, tissue plasminogen activator (TPA), urokinase, hirudin, and streptokinase, antiproliferatives  
25 (methotrexate, cisplatin, 5-fluorouracil, Taxol, Adriamycin, and the like) antioxidants (ascorbic acid, carotene, B, vitamin E, and the like), antimetabolites, thromboxane inhibitors, non-steroidal and steroidal antiinflammatory drugs, Beta and Calcium channel blockers, genetic materials including DNA and RNA fragments, and complete expression genes, carbohydrates, and proteins including but not limited to antibodies (monoclonal and  
30 polyclonal) lymphokines and growth factors, prostaglandins, and leukotrienes. The sheath material may also incorporate bioactive materials such as fibronectin, laminin, elastin, collagen, and integrins. Fibronectin, for example, promotes adherence of the sheath to the tissue of the vessel 32.

35 In one specific example of a biodegradable material incorporating drugs, a  
40 25 poly-L-lactide having an intrinsic viscosity of 2.3 dl/g is used to form monofilament fibers using a spin or melt spinning process. Five percent aspirin or 5% heparin was incorporated into the melt of the poly-L-lactide prior to fiber formation. The fibers formed had a diameter of approximately 0.5 millimeters. The monofilaments were then stretched under  
45 temperatures ranging from 50° C to 200° C to orient the fiber. The temperature employed  
30 depends upon the kind of material used to make the fiber. The final diameter of the oriented fiber falls within a range of 0.1 to 0.3 millimeters. Similar processing was used to incorporate 5% aspirin or 5% heparin into poly-L-lactide and polyglycolide.

5 The device of the present invention may also include bioadhesives to be delivered to the site where the stent is needed. It is known that bioadhesives can be used to repair tissue walls. It is therefore desirable to utilize a polymer to deliver a bioadhesive to the stent implantation location. In this manner, a potential problem could be averted by the presence of the bioadhesive in the case of a tear or dissection.

10 Just as the use of a variety of biodegradable materials facilitates a controlled degradation of a biodegradable sheath according to the present invention, so similarly does the incorporation of a variety of drugs into the biodegradable materials facilitate control of drug release to perform a variety of functions. For instance, drugs released from the outer surface as the outer surface degrades facilitate adherence of the sheath to the inner surface wall 34 of the vessel 32. Drugs released from fibers perform a variety of functions, ranging from promoting cell growth to altering the blood clotting mechanisms, depending upon what drug released. In one embodiment, drugs released from the sheath as it degrades may temper platelet function in blood flowing through lumen.

15 The device of the present invention may also be used as a drug delivery system to prevent restenosis or for other treatment. The drugs may include radioactive materials to irradiate and prohibit smooth muscle cell growth. Angioplasty and stent deployment may cause injury of the endothelial cell layer of blood vessels, causing smooth muscle cell proliferation, leading to restenosis. By accelerated endothelialization on the inner wall surface of vessels will prevent or prohibit the smooth muscle growth. To stimulate endothelialization without provoking smooth muscle cell proliferation, specific growth factors may be included and delivered. Growth factors include vascular endothelial growth factor (VEGF), transforming growth factor beta (TGF $\beta$ ), insulin growth factor-1 (IGF-1), platelet derived growth factor (PDGF), basic fibroblast growth factor (bFGF), etc.

20 All such materials are referred to herein generally as "drugs" or therapeutics. These drugs may be dispersed in the matrix of the polymeric material.

25 For carrying drugs, a gel-like material may be used. The sleeve may be comprised of such a material, or it may be applied over the sleeve as a coating. There are several ways to apply drugs to such materials. The first way is to mix the drug with the materials, then form a sleeve therefrom. Alternatively the mixture may coated onto a sleeve. The gel-like materials can be cast as film or sheet with drug together, then formed into a sleeve or laminated to a sleeve.

5 Another way is to form a sleeve from a gel-like material without a drug, or to coat or laminate a polymeric sleeve with a gel-like material without the drug. The sleeve is made, and then sterilized. Due to the gel-like nature, the sleeve can then be inserted into  
10 a drug solution. The drug will be absorbed into/onto the gel.

5 The resulting drug-carrying sleeve can then be mounted to a stent and delivered into the body. The drug will then be released.

15 In one embodiment of the invention, the sleeve may be made of polyethylene oxide containing Taxol or coated with such a material. Other materials that may be used are copolymers such as PGA/PLA, PEO/PLA or the like containing a drug  
10 such as Taxol or heparin.

20 Preferred gel-like materials for use as a drug delivery sleeve or coating for a stent when drug delivery is desired are polyethylene oxide, polyvinyl pyrrolidone, polyacrylates, and their blends or copolymers or lightly cross linked forms. Polyethylene glycol block copolymer with polylactides or other polyesters are examples. Hydrophilic  
25 polyurethane, poly(maleic anhydride-alt-ethylene) and their derivatives are examples. Other materials are polysaccharides and their derivatives. There are also sodium alginate, karaya gum, gelatin, guar gum, agar, algin carrageenans, pectin, locust bean gums, xanthan,  
30 starch-based gums, hydroxy alkyl and ethyl ethers of cellulose, sodium carboxymethyl cellulose. Some of the materials will be heated, then cooled, then a gel is formed. Some  
20 of the above are food gels. Some of them are bioadhesives.

35 Any drugs may be used, singly or in combination. For example, the drugs can be an anticoagulant, e.g. aspirin, ticlopidine, an RGD peptide-containing compound, heparin, antithrombin compounds, platelet receptor antagonists, antibodies, urokinase, prostaglandin inhibitors, platelet inhibitors, or antiplatelet peptide. The drug can be an  
40 25 inhibitor of vascular cell growth, DNA, RNA, cholesterol-lowering agents, vasodilating agents. The drug can be any drug such as Taxol, 5-fluorouracil, Beta-Estradiol, Tranilast, Trepidil, Probucol, Angiopeptin or any combination of them.

45 Since there are many drugs and many polymers, the sleeve can have multiple layers of different polymers with the same or different drugs. For example, the sleeve can  
30 have two layers of the same polymer with one layer with drug and another layer without drugs. The sleeve may have two layers of the same polymer with two different drugs as  
50 another example.

5 In particular, various combinations of a cyclin kinase inhibitor identified as p21 and the vascular endothelial growth factor identified as VEGF, an endothelial nitrogen, may preferably be included in and dispensed from the sleeve or coating provided thereon.

10  
15  
20  
25  
30  
35  
40  
45  
50  
55  
Incorporation of drugs and growth factors into the sleeve material or coating thereof can also be performed by several other methods, including the solvent method, melting method, soaking method and spraying method. If both polymer and drug have a cosolvent, a solution case will be an easy way to provide the polymer matrix loaded with the drug or growth factor. If the polymer can be melted at low temperature and the drug or growth factor tolerates heating, a melting method can be used to mix the drug or growth factor into the polymer matrix. Also, a polymer-drug solution or suspension solution can be used for coating to provide a layer containing the drug or growth factor.

25  
30  
35  
40  
45  
50  
55  
In another embodiment of the invention the sleeve may be coated with a film of bioadhesive. Bioadhesives glue the tissue together. Using a bioadhesive for the coating serves two purposes. If a tear has occurred prior to or during delivery of the stent on which the sleeve is mounted, the tissue can be repaired. In this manner, blood flow will be maintained in a vessel, for example. The bioadhesive may or may not also have drugs loaded for delivery. Dissection, cutting or tearing occurs in some stent delivery and PTCA procedures. Bioadhesives or surgical adhesives may be used to repair the passage wall. However, these tears or cuts are not necessarily discovered immediately. In those cases, a further medical procedure must be undertaken to repair the wall. The need for such an additional medical procedure may be eliminated where a bioadhesive is included as a coating on the sleeve mounted to the stent which is deployed in place, as the bioadhesive will repair damage to the vessel wall. The bioadhesive is chosen as the coating for the sleeve, or is used in addition to a coating on the sleeve and is applied in a known manner to the sleeve. The end or edge, side, outside and/or inside of the sleeve may utilize the bioadhesive.

Any appropriate bioadhesive may be used. For example, the following bioadhesives may be used singly or in combination:

cyanoacrylate; ethyl cyanoacrylate, butyl cyanoacrylate, octyl cyanoacrylate, hexyl cyanoacrylate;

fibrin glue: fibrinogen/thrombin/Factor XIII/calcium as catalyst

5 gelatin-resorcinol-formol (GRF) glue: formed from gelatin, resorcinol and  
water in the presence of formaldehyde, glutaraldehyde and heat (45°C);

10 mussel adhesive protein, prolamine gel and transforming growth factor  
beta(TGF-B);

5 polyacrylic acid, modified hydrocellulose, hydroxypropylmethyl cellulose,  
hydroxypropylcellulose, carboxymethyl cellulose, sodium alginate, gelatin, pectin,  
polyvinylpyrrolidone, polyethylene glycol, aldehyde relative multifunctional chemicals,  
15 polyallylsaccharose, and polypeptides.

Suitable materials for the device of the present invention and suitable drugs  
10 to be delivered thereby are also set forth in U.S. Application No. 08/874,190.

20 Although the present invention has been described with reference to  
preferred embodiments, workers skilled in the art will recognize that changes may be made  
in form and detail without departing from the spirit and scope of the invention.

25 The above Examples and disclosure are intended to be illustrative and not  
15 exhaustive. These examples and description will suggest many variations and alternatives  
to one of ordinary skill in this art. All these alternatives and variations are intended to be  
included within the scope of the attached claims. Those familiar with the art may recognize  
30 other equivalents to the specific embodiments described herein which equivalents are also  
intended to be encompassed by the claims attached hereto.

20 F:\WPWORK\WEA\8471-APP.831

## Claims

5

10

15

20

25

30

35

40

45

50

55

WHAT IS CLAIMED IS:

What is claimed is:

1. An implantable intraluminal apparatus comprising in combination:  
an expandable intraluminal stent comprising a main body portion having a first end  
portion, a second end portion, a middle portion, an exterior surface and an interior flow  
passage defined therethrough; and  
a sheath constructed and arranged for mounting on the stent for delivery of drugs  
to an implanted site, said sheath comprising a biocompatible polymeric material and a drug  
carried thereby.
2. The apparatus of claim 1 wherein the sheath comprises polyurethane.
3. The apparatus of claim 1 wherein the sheath comprises polytetrafluoroethylene.
4. The apparatus of claim 1 wherein the sheath comprises a gel-like material.
5. The apparatus of claim 1 wherein the sheath comprises a cellulose polymer.
6. The apparatus of claim 1 wherein the sheath comprises a biodegradable polymer.
7. The apparatus of claim 1 wherein the sheath comprises poly(N-vinyl-2-pyrrolidone).
8. The apparatus of claim 1 wherein the sheath comprises polyethylene oxide.
9. The apparatus of claim 1 wherein the drug is selected from the group consisting of  
pharmaceutical agents, radioactive agents, bioactive agents and combinations thereof.
11. The apparatus of claim 1 wherein the drug is selected from the group consisting of  
TAXOL, vascular endothelial growth factor, heparin, 5-fluorouracil, beta-estradiol,  
tranilast, trapidil, probucol, and angiopeptin.
12. The apparatus of claim 1 wherein the sheath is cylindrical.
13. The apparatus of claim 1 wherein the sheath further comprises a proximal end, a  
distal end and a slit extending from the proximal end to the distal end.
14. The apparatus of claim 13 wherein the slit is a longitudinal slit.
15. The apparatus of claim 13 wherein the slit is helical.
16. The apparatus of claim 1 wherein the sheath is a helical coil.
17. The apparatus of claim 1 wherein the sheath comprises a plurality of layers.
18. The apparatus of claim 17 wherein the plurality of layers is comprised of the same  
material.
19. The apparatus of claim 17 wherein the plurality of layers is comprised of different  
materials.


- 5                   20.    The apparatus of claim 17 wherein at least one of the layers includes a drug.
21.    The apparatus of claim 1 wherein the sheath further comprises an inner surface, an  
10                   outer surface, and a coating covering at least a portion of the outer surface thereof.
- 5                   22.    The apparatus of claim 21 wherein the coating comprises a biocompatible polymer.
23.    The apparatus of claim 21 wherein the coating comprises polyethylene oxide.
24.    The apparatus of claim 21 wherein the coating comprises polyurethane.
- 15                   25.    The apparatus of claim 21 wherein the coating comprises a gel-like material.
26.    The apparatus of claim 21 wherein the drug is carried by the coating.
- 10                   27.    The apparatus of claim 21 wherein the coating includes a bioadhesive.
- 20                   28.    The apparatus of claim 27 wherein the bioadhesive is selected from the group  
                  consisting of cyanoacrylate, fibrin glue, gelatin-resorcinol-formol glue.
29.    The apparatus of claim 21 wherein the coating comprises a plurality of layers.
- 25                   30.    The apparatus of claim 29 wherein the plurality of layers is comprised of the same  
15                   coating material.
31.    The apparatus of claim 29 wherein the plurality of layers is comprised of different  
                  coating materials.
- 30                   32.    The apparatus of claim 29 wherein at least one of the layers includes a drug.
33.    An implantable intraluminal apparatus comprising:  
20                   a sheath constructed and arranged for mounting on a stent for delivery of drugs to  
                  an implanted site, said sheath comprising a biocompatible polymeric material and a drug  
35                   carried thereby.
34.    A sheath constructed and arranged for mounting on a stent for delivery of drugs to  
                  an implanted site, said sheath comprising a biocompatible polymeric material and a drug  
40                   25                   carried thereby.
35.    A sheath for an implantable intraluminal apparatus for delivery of a stent, the sheath  
                  constructed and arranged for mounting on a stent for delivery of drugs to an implanted site,  
45                   said sheath comprising a biocompatible polymeric material and a drug carried thereby.
36.    A sheath for being delivery into the body with a stent, the sheath constructed and  
30                   arranged for mounting on a stent for delivery of drugs to an implanted site, said sheath  
                  comprising a biocompatible polymeric material and a drug carried thereby.
- 50
- 55




5 37. A drug delivery sheath for delivering drugs within the body, the sheath constructed  
and arranged for being associated with a stent for delivery of drugs to an implanted site,  
said sheath comprising a biocompatible polymeric material and a drug carried thereby.

10 38. A sheath constructed and arranged for being introduced within the body for delivery  
5 of drugs to an implanted site, said sheath comprising a biocompatible polymeric material  
and a drug carried thereby.


15  
10

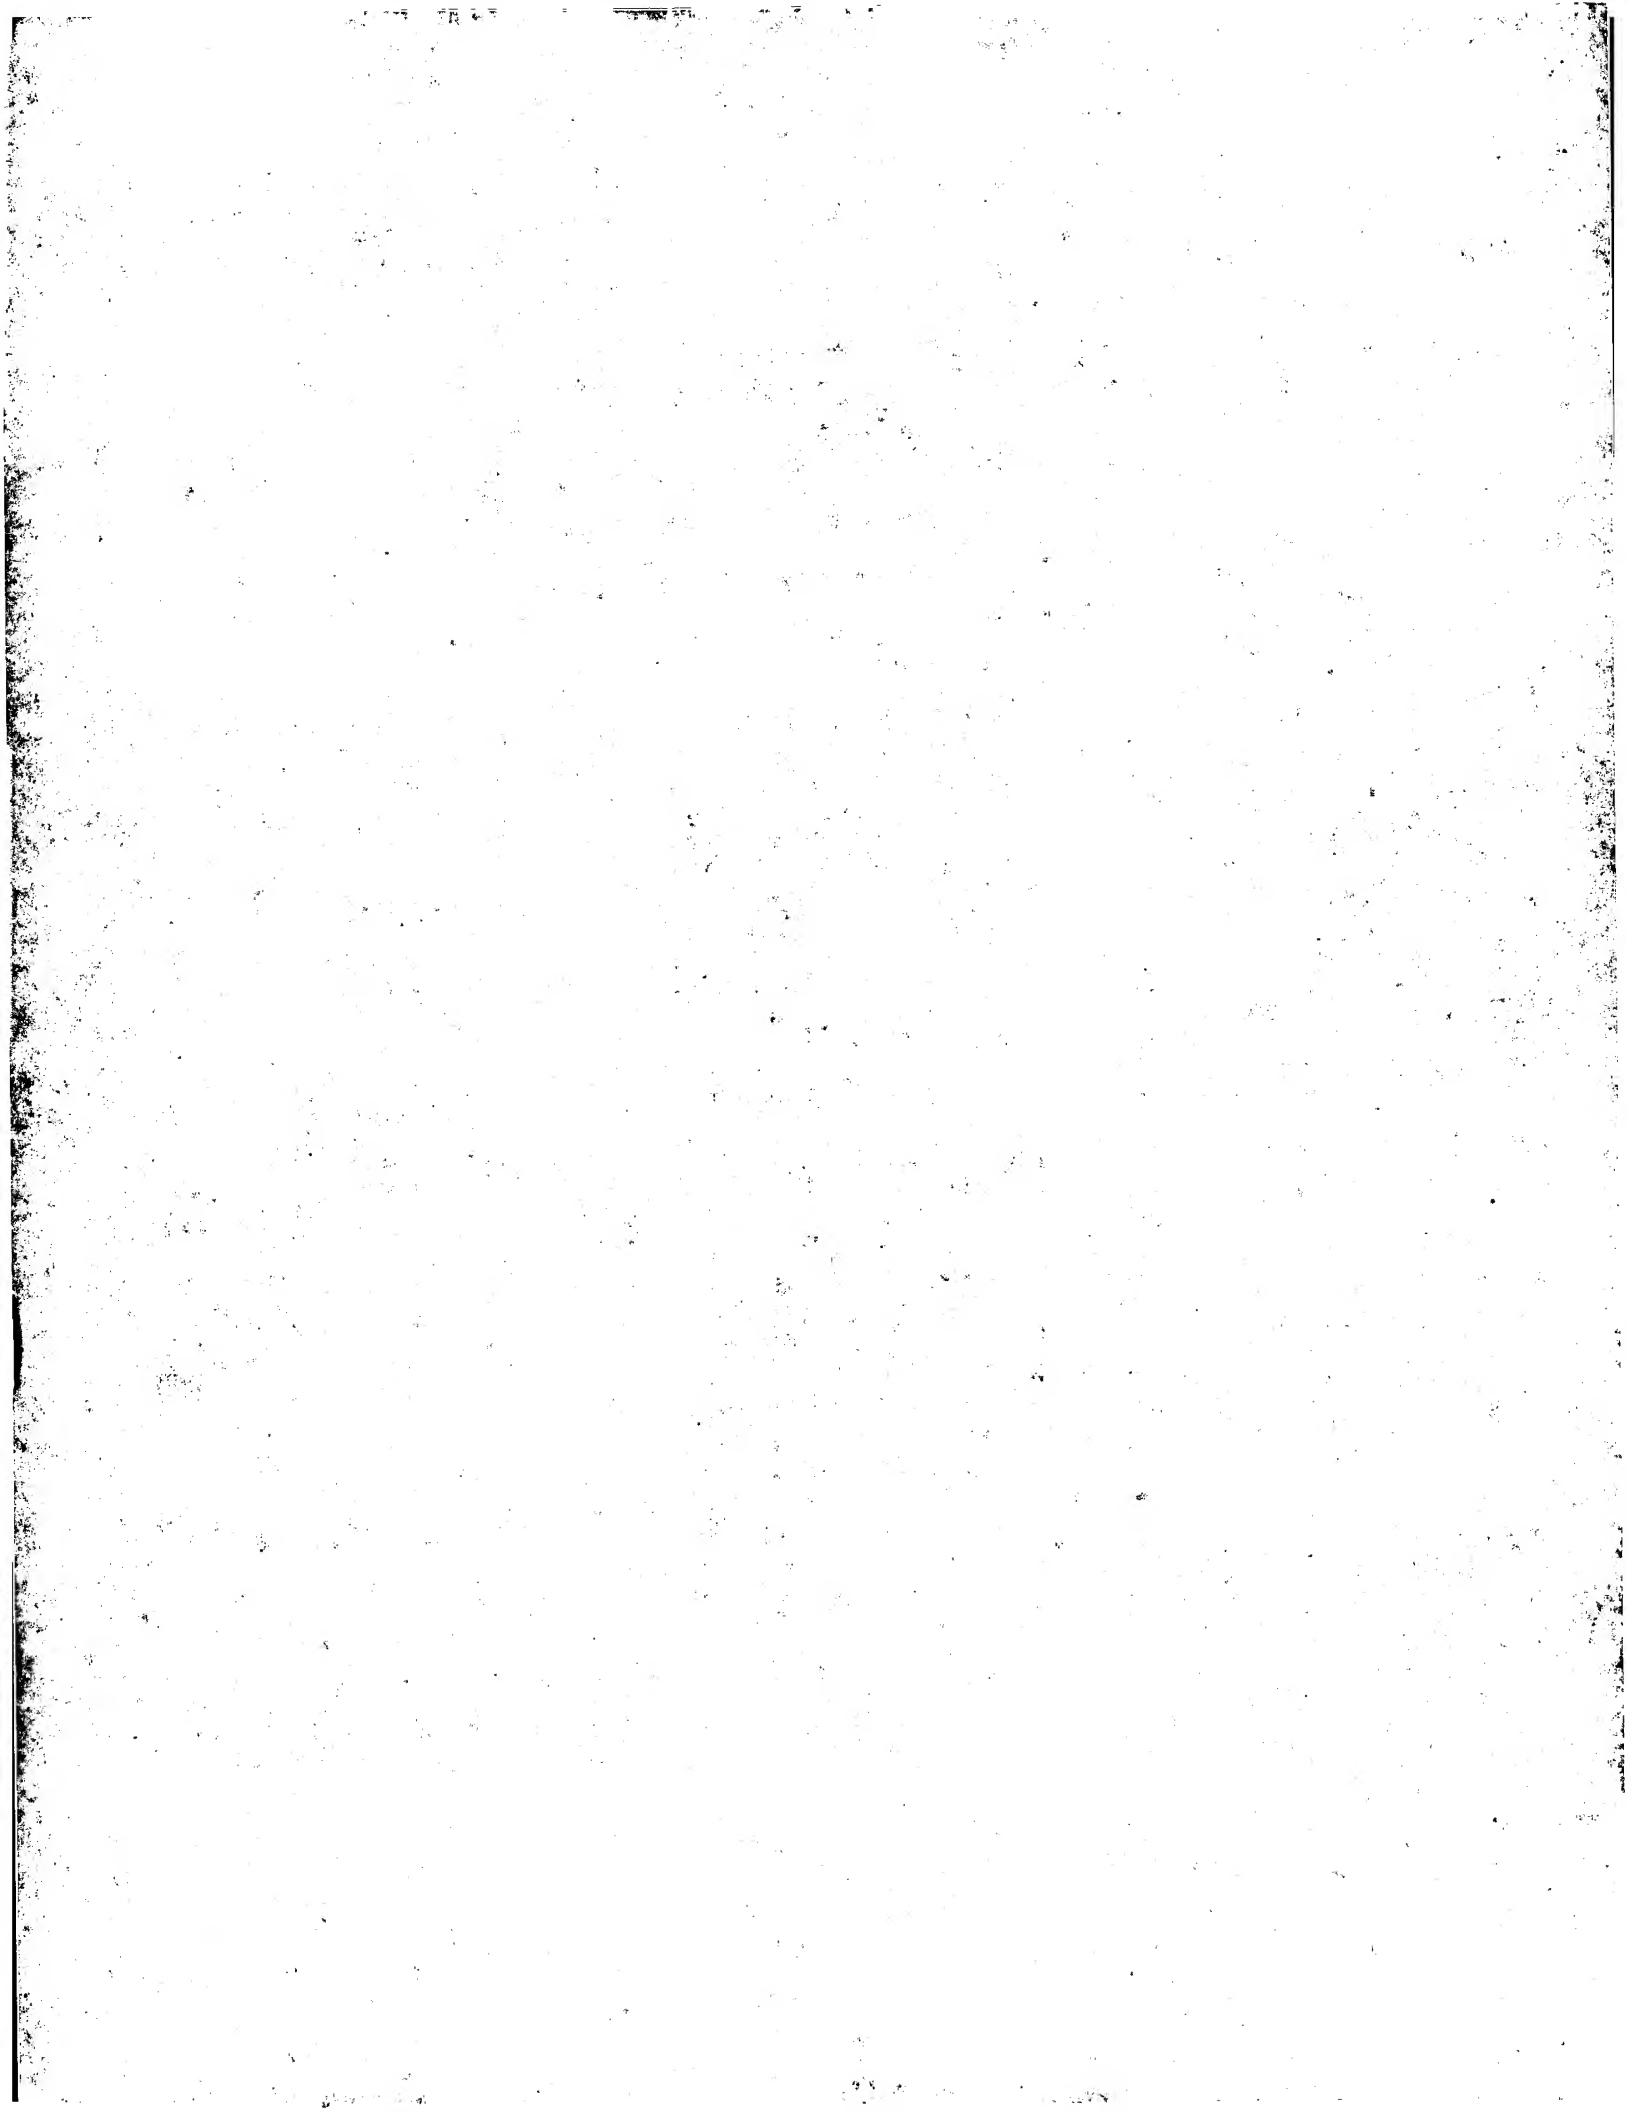


*Fig. 1*

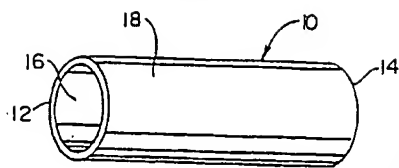

*Fig. 2a*

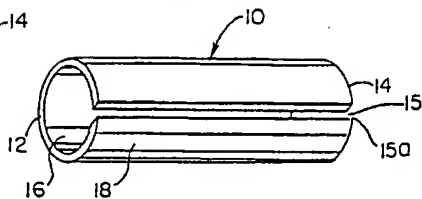


*Fig. 3*

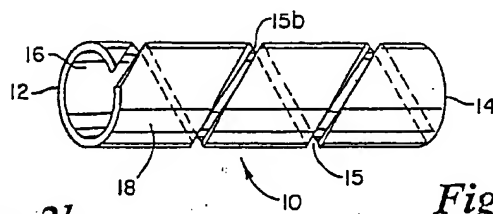


*Fig. 7*




*Fig. 2b*




*Fig. 4*

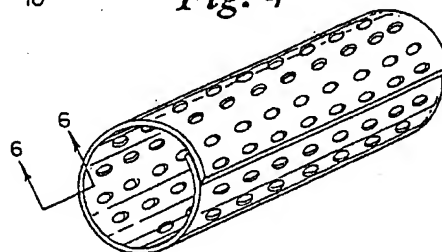

*Fig. 5*




*Fig. 6*







*Fig. 8*

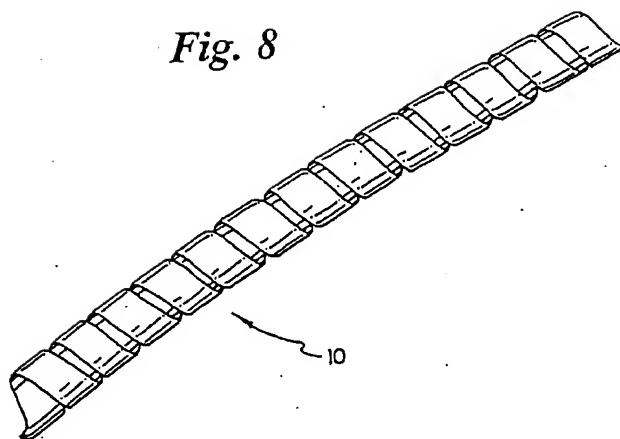


*Fig. 9*

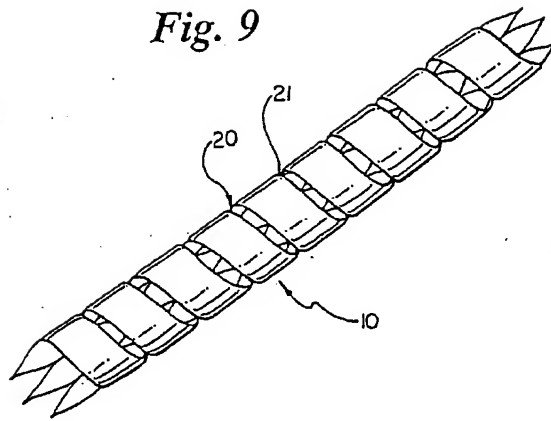

*Fig. 10*

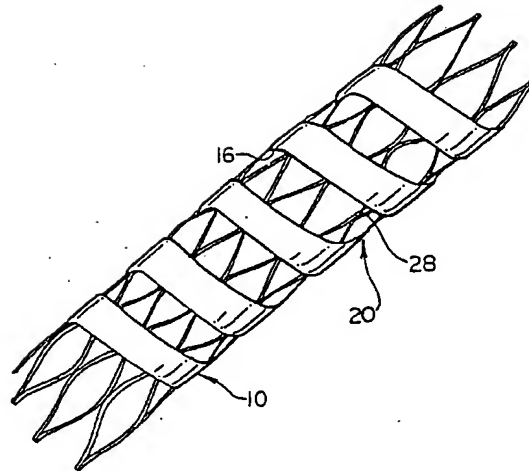

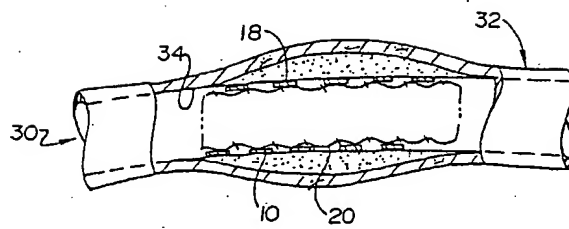*Fig. 11*




# INTERNATIONAL SEARCH REPORT

Int. l. Application No  
PCT/US 99/19697

A. CLASSIFICATION OF SUBJECT MATTER		
IPC 7	A61L31/08	A61L31/16 A61L31/18 A61K51/12 A61F2/06
According to International Patent Classification (IPC) or to both national classification and IPC		
B. FIELDS SEARCHED		
Minimum documentation searched (classification system followed by classification symbols)		
IPC 7 A61L A61K A61F		
Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched		
Electronic data base consulted during the international search (name of data base and, where practical, search terms used)		
C. DOCUMENTS CONSIDERED TO BE RELEVANT		
Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 5 383 928 A (SCOTT NEAL A ET AL) 24 January 1995 (1995-01-24) claims; figure 3	1-38
X	EP 0 716 836 A (ADVANCED CARDIOVASCULAR SYSTEM) 19 June 1996 (1996-06-19) claims; figures	1-38
X	EP 0 712 615 A (ADVANCED CARDIOVASCULAR SYSTEM) 22 May 1996 (1996-05-22) claims	1-38
X	EP 0 604 022 A (ADVANCED CARDIOVASCULAR SYSTEM) 29 June 1994 (1994-06-29)  claims	1, 6, 9, 11, 17-22, 26, 29-38
-/-		
<input checked="" type="checkbox"/> Further documents are listed in the continuation of box C. <input checked="" type="checkbox"/> Patent family members are listed in annex.		
* Special categories of cited documents: "A" document defining the general state of the art which is not considered to be of particular relevance "E" earlier document but published on or after the international filing date "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified) "O" document referring to an oral disclosure, use, exhibition or other means "P" document published prior to the international filing date but later than the priority date claimed "T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention "X" document of particular relevance: the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone "Y" document of particular relevance: the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art "Z" document member of the same patent family		
Date of the actual completion of the international search		Date of mailing of the international search report
18 January 2000		25/01/2000
Name and mailing address of the ISA European Patent Office, P.B. 5818 Patentlaan 2 NL - 2280 HV Rijswijk Tel. (+31-70) 340-2040, Tx. 31 651 epo nl, Fax: (+31-70) 340-3018		Authorized officer  ESPINOSA, M

Form PCT/ISA/210 (second sheet) (July 1992)

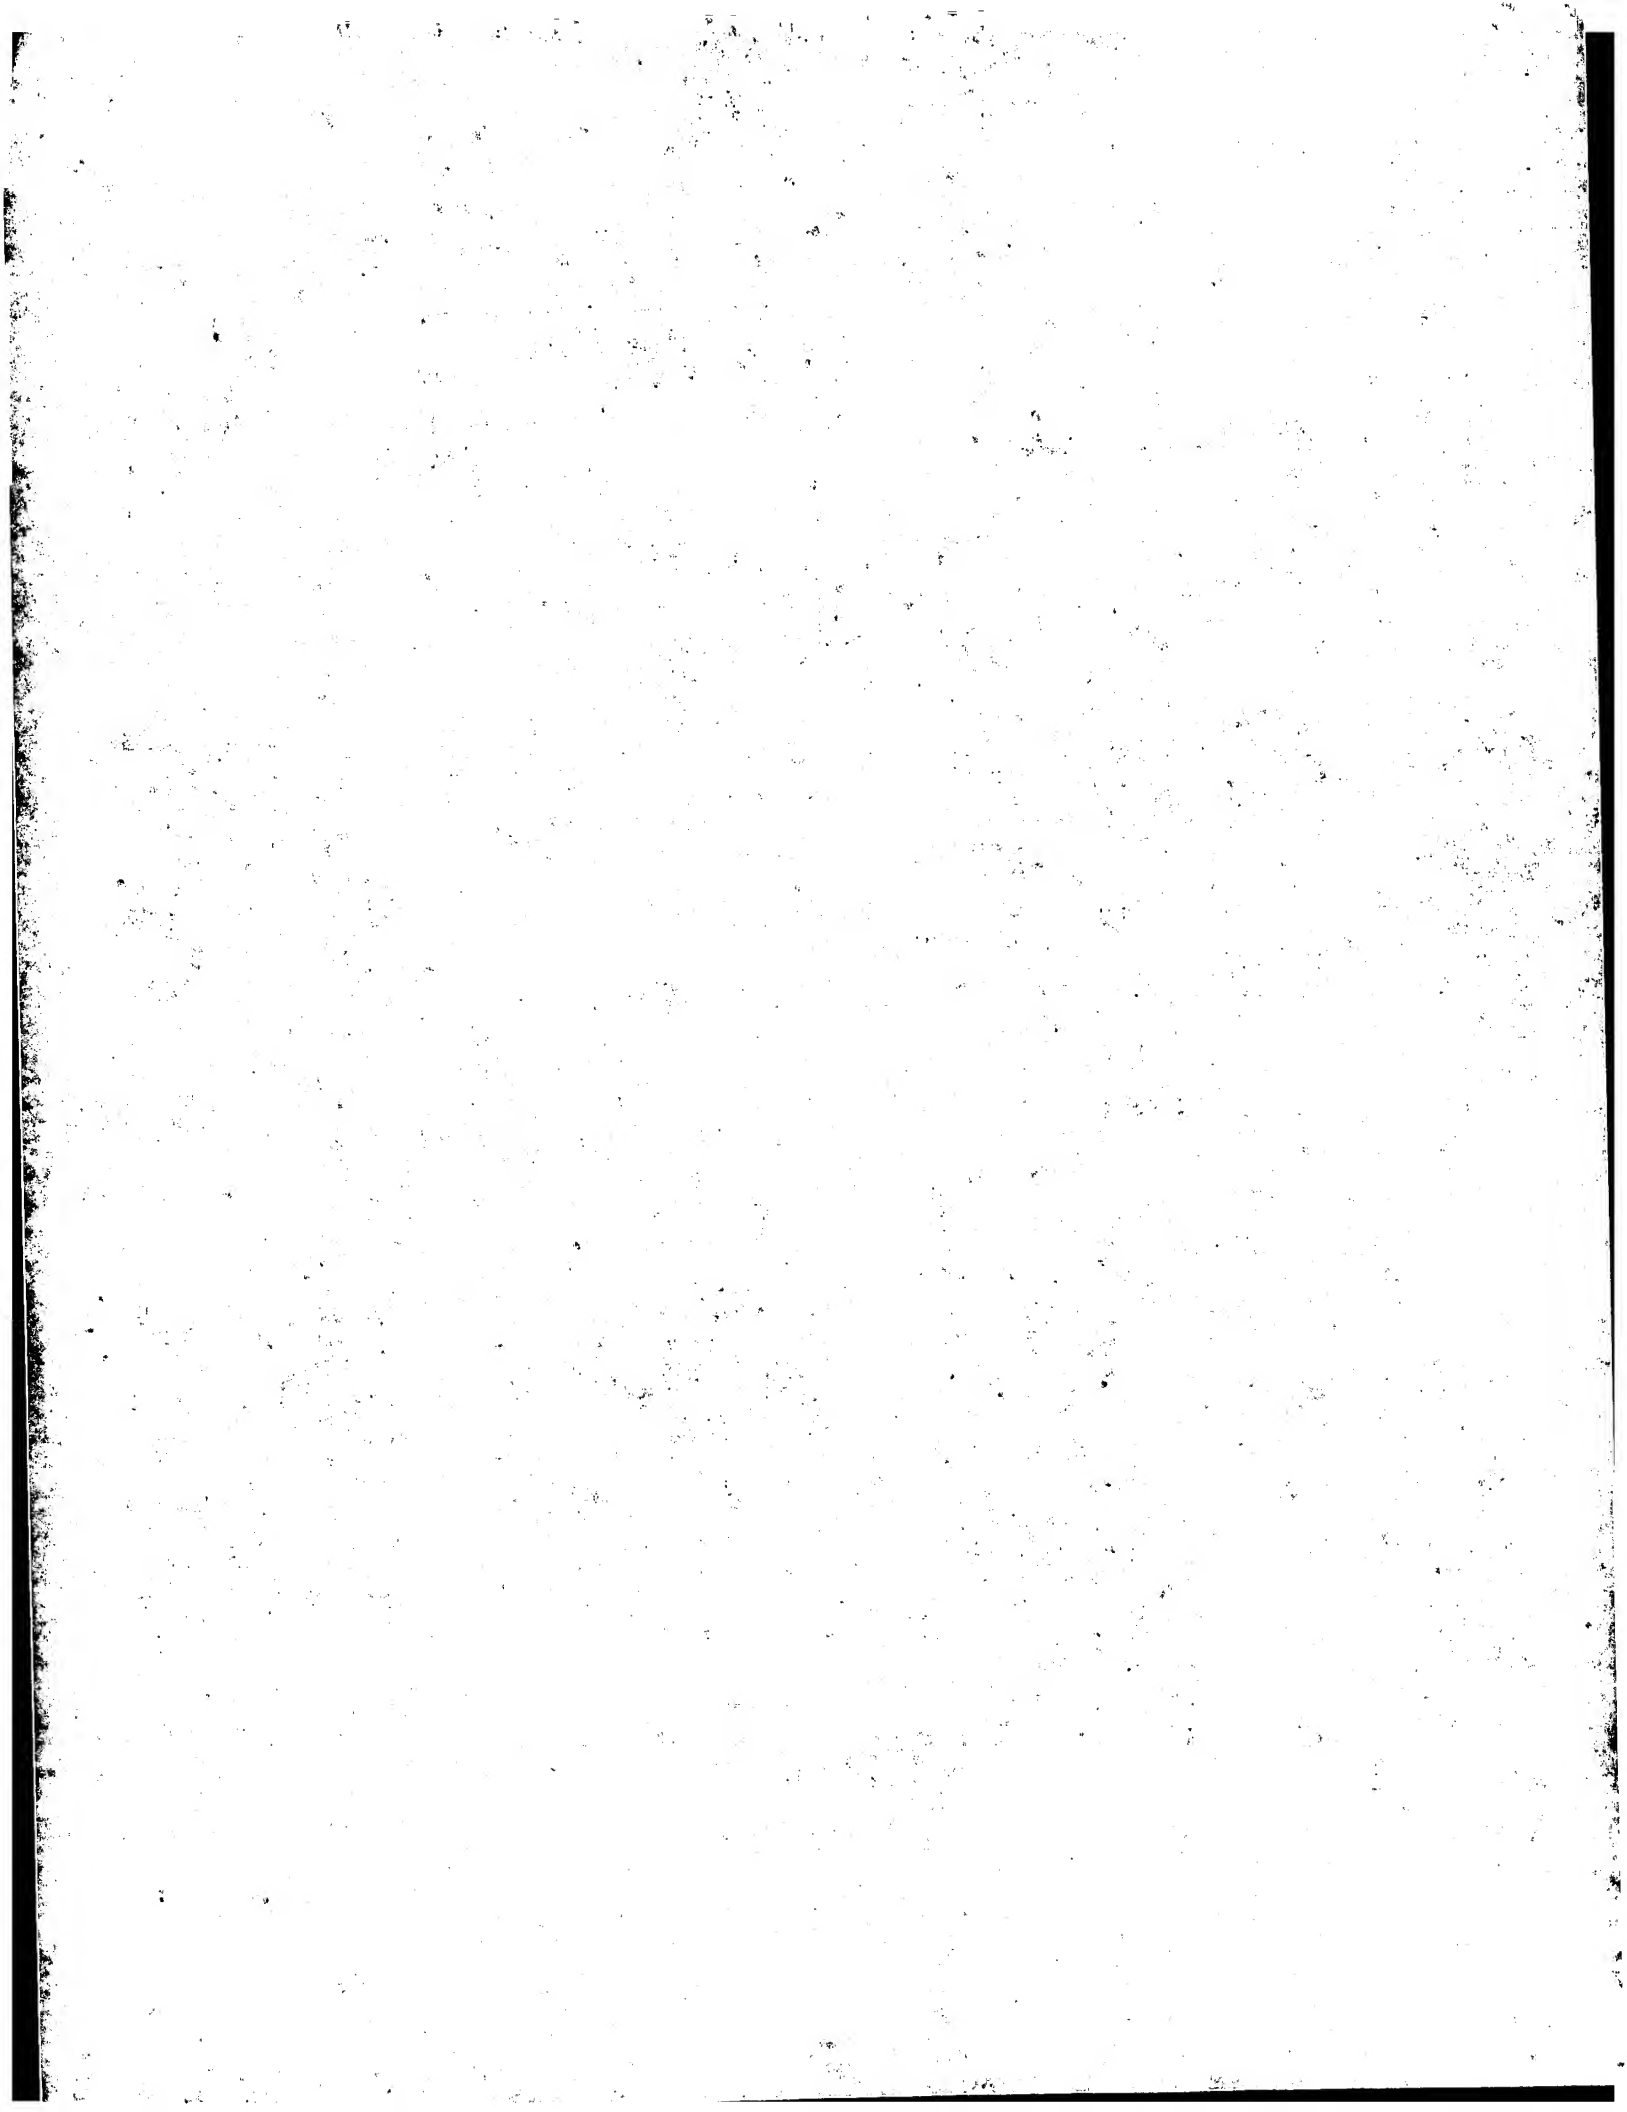


## INTERNATIONAL SEARCH REPORT

International Application No.  
PCT/US 99/19697

## C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	EP 0 578 998 A (STRECKER ERNST PETER DR MED PR) 19 January 1994 (1994-01-19) claims ---	1,4,6,9, 11
X	WO 95 29647 A (SCIMED LIFE SYSTEMS INC) 9 November 1995 (1995-11-09) claims; figures ---	1,4,6,9, 11
X	US 5 578 075 A (DAYTON MICHAEL P) 26 November 1996 (1996-11-26) claims; figures ---	1,9,11
X	WO 96 25176 A (RENO JOHN M ;KUNZ LAWRENCE L (US); NEORX CORP (US)) 22 August 1996 (1996-08-22) claims ---	1,9,11
X	WO 98 36784 A (COOK INC) 27 August 1998 (1998-08-27) claims ---	1
A	WO 93 06792 A (SCIMED LIFE SYSTEMS INC) 15 April 1993 (1993-04-15) figures ---	1-38

Form PCT/ISA/210 (continuation of second sheet) (July 1992)

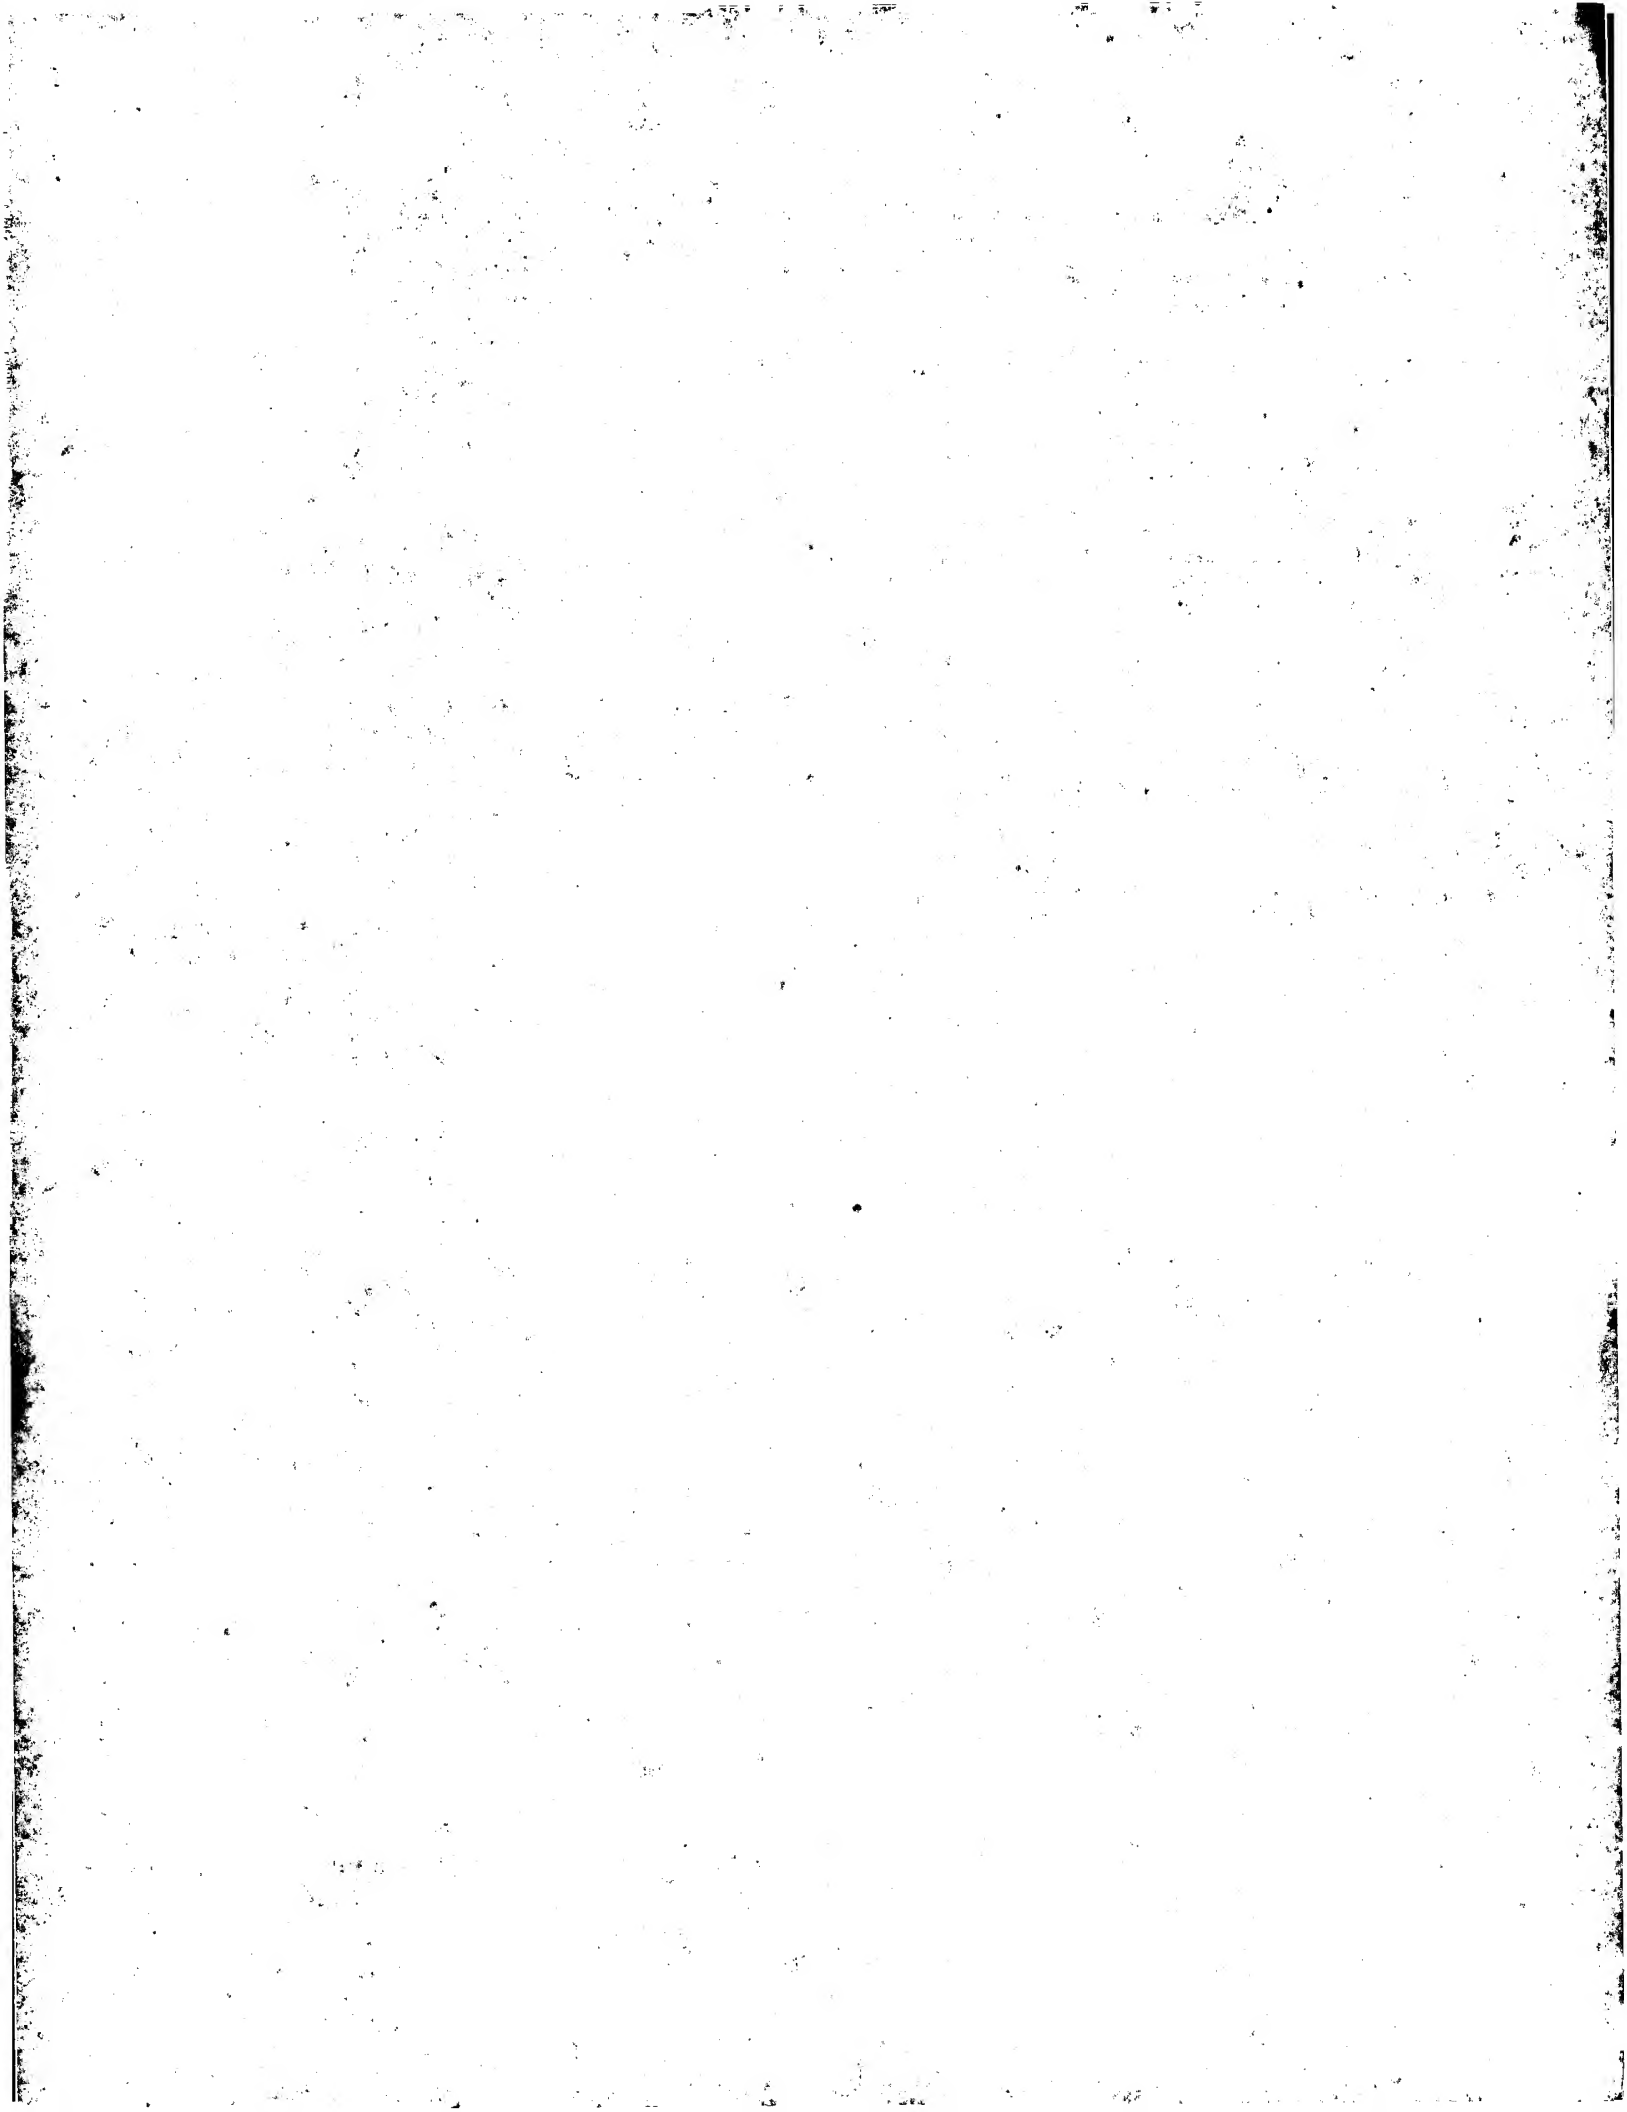

# INTERNATIONAL SEARCH REPORT

Information on patent family members

Initial Application No

PCT/US 99/19697

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 5383928 A	24-01-1995	NONE	
EP 0716836 A	19-06-1996	US 5637113 A AU 4031295 A CA 2164684 A JP 8224297 A US 5700286 A	10-06-1997 20-06-1996 14-06-1996 03-09-1996 23-12-1997
EP 0712615 A	22-05-1996	US 5707385 A AU 3783395 A AU 7010498 A CA 2162969 A JP 8317993 A	13-01-1998 23-05-1996 30-07-1998 17-05-1996 03-12-1996
EP 0604022 A	29-06-1994	CA 2111455 A JP 6218063 A	23-06-1994 09-08-1994
EP 0578998 A	19-01-1994	DE 4222380 A AT 158941 T DE 59307482 D ES 2107588 T JP 6205838 A	13-01-1994 15-10-1997 13-11-1997 01-12-1997 26-07-1994
WO 9529647 A	09-11-1995	EP 0746375 A EP 0754017 A JP 9503945 T JP 10503663 T WO 9511055 A US 5693085 A	11-12-1996 22-01-1997 22-04-1997 07-04-1998 27-04-1995 02-12-1997
US 5578075 A	26-11-1996	US 5449382 A	12-09-1995
WO 9625176 A	22-08-1996	AU 4985196 A CA 2212537 A EP 0809515 A JP 11500635 T US 5981568 A	04-09-1996 22-08-1996 03-12-1997 19-01-1999 09-11-1999
WO 9836784 A	27-08-1998	AU 6663298 A EP 0968013 A	09-09-1998 05-01-2000
WO 9306792 A	15-04-1993	US 5968092 A US 5464450 A US 5551954 A US 5500013 A US 5769883 A	19-10-1999 07-11-1995 03-09-1996 19-03-1996 23-06-1998

